


Fig. 1

2044720" 096E200T

File: Carboxy KMAPP, ID: Carboxy KMAPP

Date: 02/08/01 12:49 Step: 0.050° Cent Time: 1.000 s o.

Range: 2.00 - 40.00 (Deg) Cent. Scan Rate: 3.00 Deg/min. TQVA

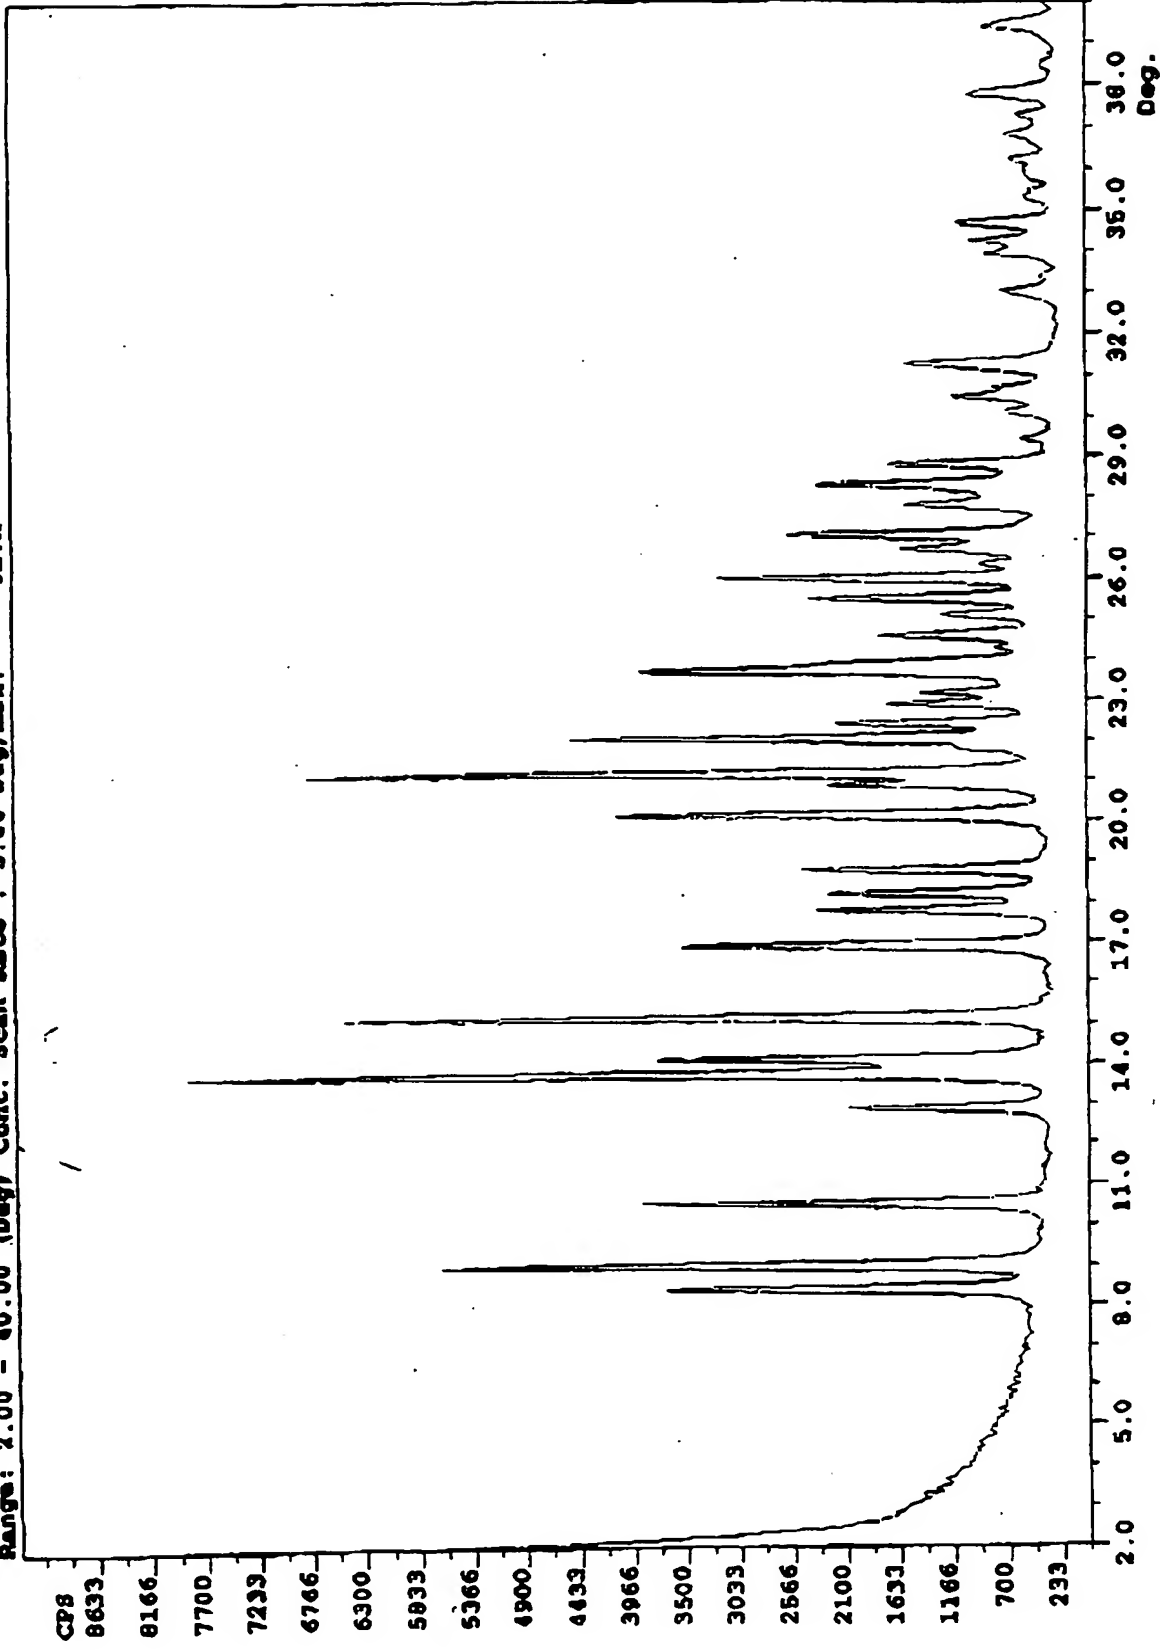

KENYON & KENYON (202) 220-4200

Inventor: L. METZGER ET AL.

Serial No.: TO BE ASSIGNED

Filed: February 14, 2002

Group Art Unit: To be assigned

Sheet: 1 of 2

Docket #: 1662/56202

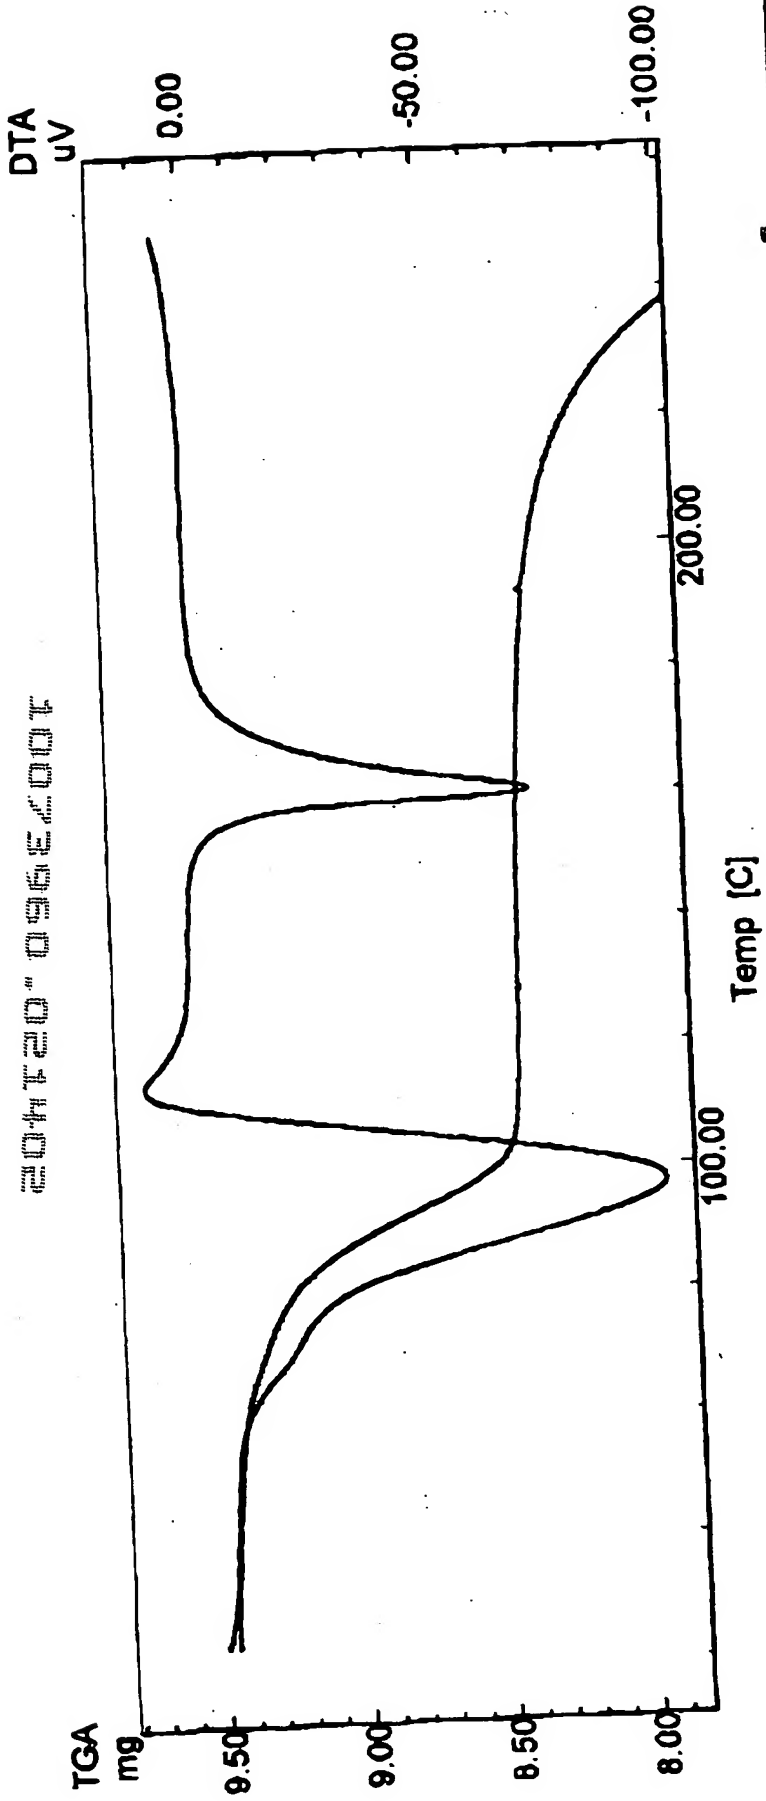


fig 2

KENYON & KENYON (202) 220-4200

Inventor: L. METZGER ET AL.

Serial No.: TO BE ASSIGNED

Filed: February 14, 2002

Group Art Unit: To be assigned

Sheet: 2 of 2

Docket #: 1662/56202